
the FAST TRACK to your ablation delivery in a single solution

VersaCross™ Workflow


Mechanical Needle Workflow

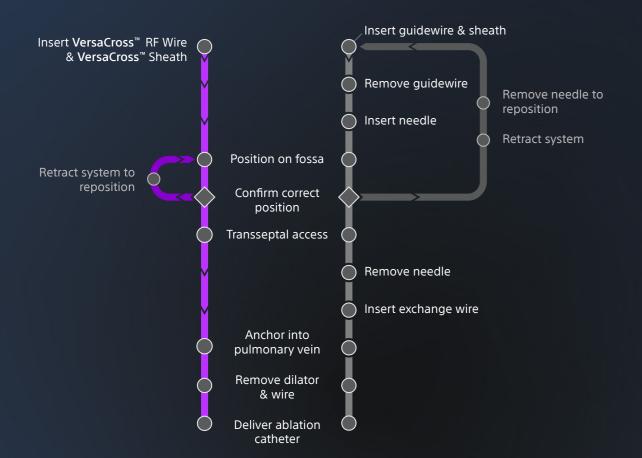

VersaCross™ RF Transseptal Solution

Full platform of tools to personalize your solution


PERSONALIZE YOUR SOLUTION

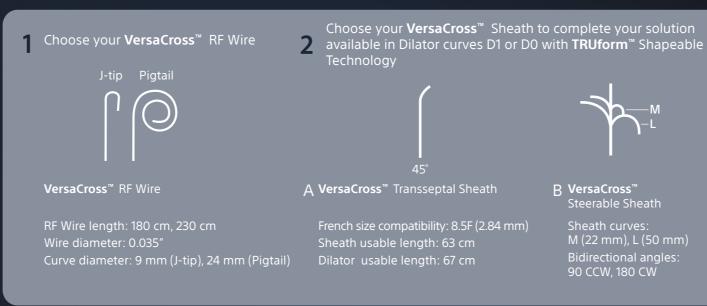





J-tip wire also available



Eliminate exchanges



Access with precision



Secure effortless delivery



I trademarks are property of their respective owners. Patents Pending and/or issued. Caution: The law restricts these devices to sale by or on the order of a physician. Indications, Contraindications, Warnings, and Instructions For Use can be found in the product labelling supplied with each device at www.baylismedical.com.

roducts shown for INFORMATION purposes only and may not be approved or for sale in certain countries. This material not intended for use in France.




© 2023 Boston Scientific Corporation or its affiliates. All rights reserved.

EP-1559409-AA



Deliver left heart ablation devices with ease






the only EXCHANGELESS* solution for access-to-delivery of left heart ablation devices

ELIMINATE EXCHANGES

Left heart access using a SINGLE SOLUTION from start to finish







Drop down to optimize transseptal location WITHOUT THE HASSLE of exchanging a needle

*VersaCross™ RF Wire can be used, without exchanges, as a guidewire, as a transseptal puncture device or as an exchange rail for delivering therapy sheaths.

VERSATILITY

INSTANTLY SECURE ACCESS

RF Puncture Technology allows crossing even in challenging anatomy. Instantly probe and anchor into pulmonary vein without exchanges.



Shapeable dilator with true-to-form curve retention



DELIVER CONSISTENT CONTACT FORCE[†]

Retain your curve and support consistent contact force[†] with the **VersaCross**™ Steerable Sheath. Consistent contact force of ablation catheters provides better therapeutic results.¹

TruGlide[™]

RESPONSIVE HANDLING
Responsive,

smooth, highprecision steering to confidently position your curve †Assessed by repeated bit curve radius at each step maximal extension up to Comparisons done using and dilator inside sheath Steerable Guiding Sheatl VersaCross™ Steerable S may not necessarily be in performed by or on behal


rmed by or on behalf of Boston Scientific. Data on file.

Know where you are at all times with

OMNIviz[™] Technology



Track and mark RF tip position on your mapping system



Reliably locate your devices on ultrasound to reduce reliance on fluoroscopy



Visualize your entire solution on fluoroscopy



Visibly confirm position of RF tip within dilator

VersaCross[™]
RF Transseptal Solution