

ZERO EXCHANGE

to your therapy delivery
in a SINGLE SOLUTION



VersaCross Connect™

Access Solution for FARADRIE™

DESIGNED for use with the
FARADRIE™
Steerable Sheath†

**3-IN-1
RF WIRE**
for use as a starter wire,
puncture device, and
exchange rail



Smooth transition between
VersaCross Connect™ Dilator
and FARADRIE™ Sheath†

Snap-lock designed for
FARADRIE™ Sheath†

†FARADRIE™ Steerable Sheath as shown in this brochure is sold separately.

VersaCross™ RF Wire

CAUTION: Federal law (USA) restricts this device to sale by or on the order of a physician. Rx only. Prior to use, please see the complete "Instructions for Use" for more information on Indications, Contraindications, Warnings, Precautions, Adverse Events, and Operator's Instructions.

INDICATIONS FOR USE: The VersaCross™ RF Wire is indicated for creation of an atrial septal defect in the heart.

CONTRAINDICATIONS: The VersaCross™ RF Wire is not recommended for use with any conditions that do not require the creation of an atrial septal defect. The Connector Cable is not recommended for use with any other Baylis RF Generator or any other device.

WARNINGS: • Laboratory staff and patients can undergo significant x-ray exposure during RF puncture procedures due to the continuous usage of fluoroscopic imaging. This exposure can result in acute radiation injury as well as increased risk for somatic and genetic effects. Therefore, adequate measures must be taken to minimize this exposure. • The VersaCross™ RF Wire and Connector Cable are intended for single patient use only. Do not attempt to sterilize and reuse either device. Reuse can cause patient injury and/or the communication of infectious disease(s) from one patient to another. Reuse may result in patient complications. • The VersaCross™ RF Wire must be used with the Connector Cable provided. Attempts to use it with other connector cables can result in electrocution of the patient and/or operator. • Do not use the VersaCross™ RF Wire with electrocautery or electrosurgery generators, connector cables or accessories as attempted use can result in patient and/or operator injury. • The Connector Cable must only be used with the RFP-100A Baylis RF Generator and the included VersaCross™ RF Wire. Attempts to use it with other RF Generators and devices can result in electrocution of the patient and/or operator. • The VersaCross™ RF Wire must be used with 0.035" compatible transeptal sheath and/or dilator devices. Use of incompatible accessory devices may damage the integrity of the VersaCross™ RF Wire or accessory devices and may cause patient injury. • The VersaCross™ RF Wire has only been validated for transeptal puncture use through VersaCross™ dilators which have been demonstrated to provide the required support for optimal function. • The VersaCross™ RF Wire is not intended for use with neonatal patients (i.e. less than one month of age). Do not attempt to treat neonatal patients with the VersaCross™ RF Wire.

PRECAUTIONS: • In order to prevent the risk of ignition, ensure that flammable materials are not present in the room during RF power application. • Careful manipulation of the VersaCross™ RF Wire must be performed to avoid vessel trauma. If resistance is encountered, DO NOT use excessive force to advance or withdraw the VersaCross™ RF Wire or ancillary sheath and/or dilator assembly. Excessive force may lead to bending or kinking of the device limiting advancement and retraction of sheath and/or dilator device. • The Baylis RF Generator is capable of delivering significant electrical power. Patient or operator injury can result from improper handling of the VersaCross™ RF Wire and/or DIP electrode, particularly when operating the device. • During power delivery, the patient should not be allowed to come in contact with ground metal surfaces. • If using electroanatomical mapping guidance, it is recommended to use it along with alternative imaging modality in the event there is loss of visibility of the device.

ADVERSE EVENTS: Adverse events that may occur while creating an atrial septal defect include: • Tamponade • Sepsis/ Infection • Thromboembolic episodes • Vessel perforation • Atrial Fibrillation • Myocardial Infarction • Vessel spasm • Sustained arrhythmias • Atrial Flutter • Hemorrhage • Vascular thrombosis • Perforation of the myocardium • Hematoma • Allergic reaction to contrast medium • Ventricular Tachycardia • Pain and Tenderness • Arteriovenous fistula • Pericardial effusion • Tachycardia • Vascular Trauma • Additional Surgical Procedure • Wire entrapment/ entanglement • Foreign body/wire fracture EP-150471-AA

VersaCross Connect™ Transseptal Dilator

CAUTION: Federal law (USA) restricts this device to sale by or on the order of a physician. Rx only. Prior to use, please see the complete "Instructions for Use" for more information on Indications, Contraindications, Warnings, Precautions, Adverse Events, and Operator's Instructions.

INDICATIONS FOR USE: The VersaCross Connect Transseptal Dilator is used for the percutaneous introduction of various types of cardiovascular catheters and guidewires to all heart chambers, including the left atrium via transeptal perforation / puncture. **United States:** The VersaCross Connect Transseptal Dilator is indicated for use in procedures where access to the left atrium via the transeptal technique is desired.

CONTRAINDICATIONS: There are no known contraindications for this device.

WARNINGS: • Laboratory staff and patients can undergo significant x-ray exposure during interventional procedures due to the continuous usage of fluoroscopic imaging. This exposure can result in acute radiation injury as well as increased risk for somatic and genetic effects. Therefore, adequate measures must be taken to minimize this exposure. The use of echocardiography is recommended. • The VersaCross Connect Transseptal Dilator is intended for single patient use only. Failure to do so may result in patient complications. • Do not attempt to sterilize and reuse the VersaCross Connect Transseptal Dilator. Reuse can cause the patient injury and/or the communication of infectious disease(s) from one patient to another. • The VersaCross Connect Transseptal Dilator is supplied STERILE using an ethylene oxide process. Do not use if the package is damaged. • Care should be taken to ensure that all air is removed from the dilator before infusing through the proximal hub. • Care should be taken when inserting or removing the dilator from access sheaths or introducer sheaths. • Manual shaping of the distal curve shall be done with smooth motions along the curve. Do not use excessive force and/or pressure when reshaping. • Care should be taken when inserting or removing compatible guidewires from the dilator lumen. • Do not attempt direct percutaneous insertion of the dilator without a guidewire as this may cause vessel injury. • Careful manipulation must be performed to avoid cardiac damage or tamponade. Dilator advancement should be performed under imaging guidance. Fluoroscopic or echocardiographic imaging is recommended. If resistance is encountered, DO NOT use excessive force to advance or withdraw the device.

PRECAUTIONS: • Do not attempt to use the VersaCross Connect Transseptal Dilator before thoroughly reading the accompanying Instructions for Use. • The sterile barrier system and dilator should be visually inspected prior to use. Do not use if the sterile barrier integrity or device have been compromised or damaged. • Only physicians thoroughly trained in the techniques of the approach to be used should perform interventional procedures. • The VersaCross Connect Transseptal Dilator is compatible with introducer sheaths 13F or larger. • The VersaCross Connect Transseptal Dilator is for use with the 13F (4.31 mm) ID FARADRIE Steerable Sheath, which is 74cm in length. • The VersaCross Connect Transseptal Dilator is compatible with 0.035" transeptal devices and guidewires or smaller. • The VersaCross Connect Transseptal Dilator is NOT compatible with transeptal needles such as the "NRG™" Transseptal Needle.

ADVERSE EVENTS: Adverse events that may occur while using the VersaCross Connect Transseptal Dilator include: • Infection • Air embolus • Local nerve damage • Vessel trauma • Vessel spasm • Pseudoaneurysm • AV fistula formation • Atrial septal defect • Arrhythmias • Perforation and/or tamponade • Hematoma • Hemorrhage • Catheter entrapment • Embolic events • Valve damage • Pericardial/pleural effusion

97157448 (Rev. A)

*The therapy referred to here may be one of several left heart procedures that require transeptal access. Additional procedural steps and/or devices may be required to deliver the therapy. Before use, consult Instructions for Use for any devices accordingly.

†FARADRIE™ Steerable Sheath as shown in this brochure is sold separately.

‡The VersaCross Connect Transseptal Dilator is for use with a 13F ID FARADRIE™ Steerable Sheath which is 74cm in length, specifically, model: M004PF21M402 (US).

All trademarks are property of their respective owners. Patents Pending and/or issued. Caution: Federal law (USA) restricts these devices to sale by or on the order of a physician. Rx only. Prior to use, please see the complete "Instructions for Use" for more information on Indications, Contraindications, Warnings, Precautions, Adverse events, and Operator's instructions. Products shown for INFORMATION purposes only and may not be approved or for sale in certain countries.



Baylis Medical Company Inc.
5959 Trans-Canada Highway
Montreal, QC Canada H4T 1A1

www.baylismedical.com
info@baylismedical.com

General Inquiries
(514) 488-9801


© 2024 Boston Scientific Corporation or its affiliates. All rights reserved.

EP-1782905-AA



VersaCross Connect™

Access Solution for FARADRIE™

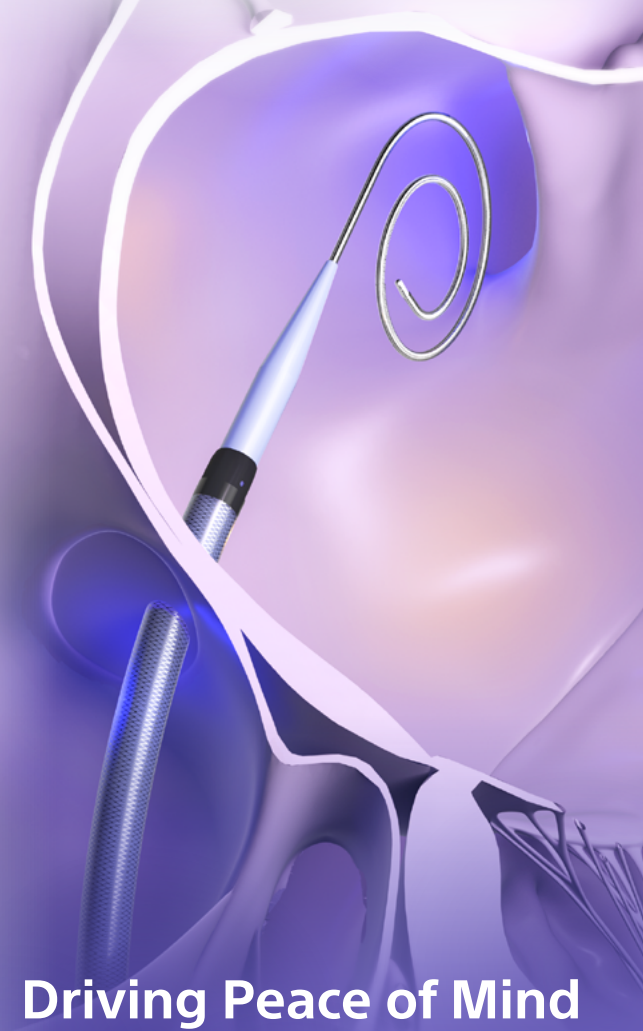

Driving Peace of Mind


ZERO EXCHANGE

FARADRIE™ Steerable Sheath delivery
For use with the FARAPULSE™
Pulsed-Field Ablation System


INTEGRATED PREDICTABILITY

with the **VersaCross Connect™** Access Solution for **FARADrive™**


EXCHANGELESS 3-in-1 RF Wire



1 Start
by tracking up to the SVC



2 Access
with purpose-built RF



3 Deliver
with confidence


Predictable and Efficient Transseptal

for smooth **FARADrive™** Steerable Sheath delivery

DELIVER THERAPY ON TARGET



TRUform™
Shapeable Technology



Precise RF
Puncture Technology



OMNIVIZ™ Technology

Reliably locate the **VersaCross Connect™** solution on fluoroscopy and ultrasound. Positional markers indicate position of RF tip within dilator. Connect to DuoMode™ Cable to track and mark RF tip on mapping systems.

VersaCross Connect™

Access Solution for **FARADrive™**

Personalize your solution

1. Choose your VersaCross™ RF Wire



2. Connect with VersaCross Connect™ Transseptal Dilator



Ordering information

Part. No.	Wire	Wire length	Dilator curve	Dilator length
VXAK0041	Pigtail	180 cm	D1	93 cm
VXAK0045	J-Tip	180 cm	D1	93 cm